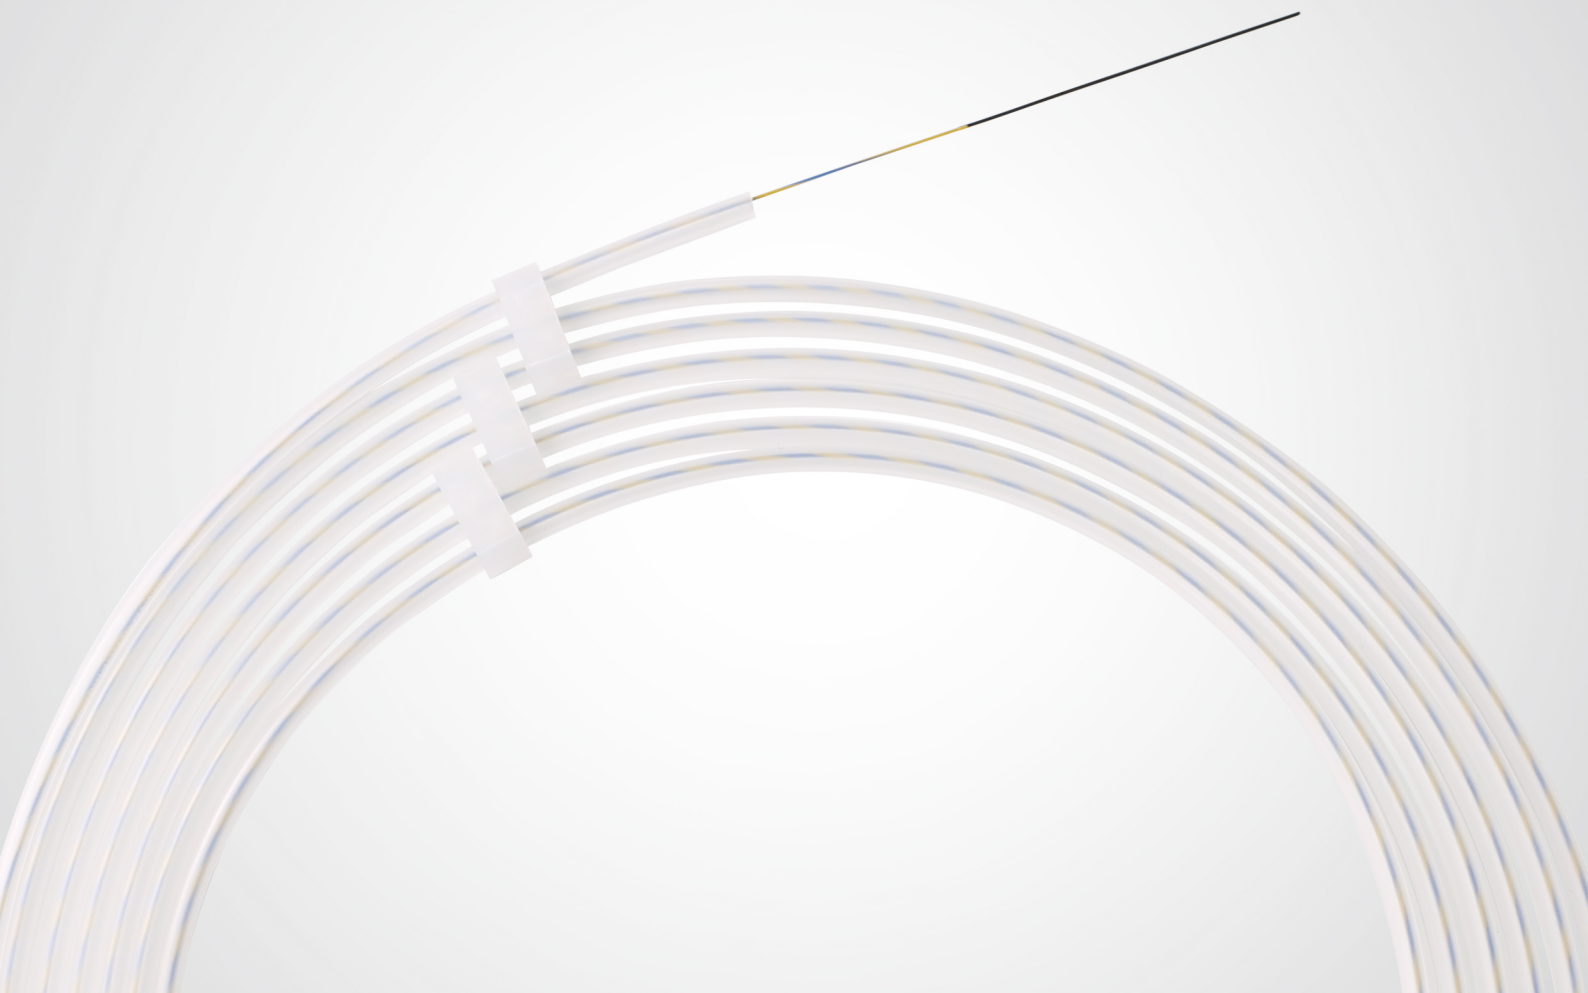


# Optimos™ Guidewire

It is used to assist in insertion of endoscopic devices for endoscopy and ultrasonography



#### HEAD OFFICE

14, Gojeong-ro, Wolgot-myeon, Gimpo-si, Gyeonggi-do, Korea 10022

#### SALES OFFICE

Bldg.C 4F, 158 Haneulmaeul-ro, ilsandong-gu, Goyang-si, Gyeonggi-do, Korea 10355  
E: [contact@stent.net](mailto:contact@stent.net) T: +82 31 904 6153 F: +82 31 904 6157





[www.taewoongmedical.com](http://www.taewoongmedical.com)



# Optimos™ Guidewire

It is used to assist in insertion of endoscopic devices for endoscopy and ultrasonography

## Ordering Information

Application	Art. No.	Wire Diameter (mm)	Distal tip Length (mm)	Total Length (mm)	Type
0.035" yellow/blue	GW3-45S	0.78	55	4500	Straight type 
	GW3-26S			2600	
	GW3-45A		60	4500	Angled type 
	GW3-26A			2600	
0.025" white/black	GW2-45S	0.61	75	4500	Straight type 
	GW2-26S			2600	
	GW2-45A		70	4500	Angled type 
	GW2-26A			2600	