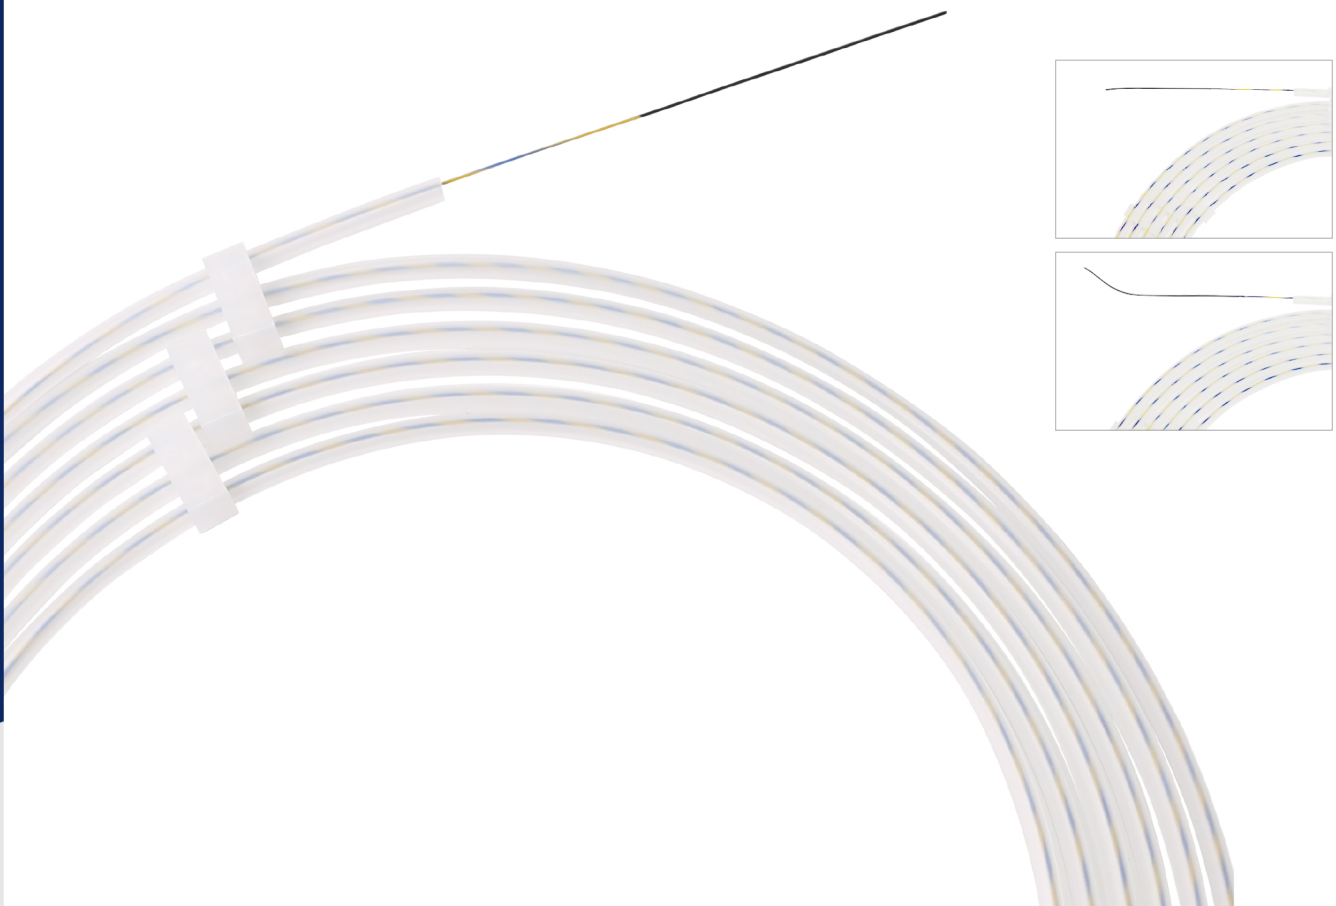


Optimos™

Guidewire

It is used to assist in insertion of endoscopic devices for endoscopy and ultrasonography



HEAD OFFICE

14, Gojeong-ro, Wolgot-myeon, Gimpo-si, Gyeonggi-do, Korea 10022



SALES OFFICE

Bldg.C 4F, 158 Haneulmaeul-ro, Ilsandong-gu, Goyang-si, Gyeonggi-do, Korea 10355
E: contact@stent.net T: +82 31 904 6153 F: +82 31 904 6157

www.taewoongmedical.com

Optimos™ Guidewire

It is used to assist in insertion of endoscopic devices
for endoscopy and ultrasonography

Ordering Information					
Application	Art. No.	Wire Diameter (mm)	Distal tip Length (mm)	Total Length (mm)	Type
0.035" yellow/blue	GW3-45S	0.78	55	4500	Straight type 
	GW3-26S			2600	
	GW3-45A		60	4500	Angled type 
	GW3-26A			2600	
0.025" white/black	GW2-45S	0.61	75	4500	Straight type 
	GW2-45A		70	4500	Angled type 